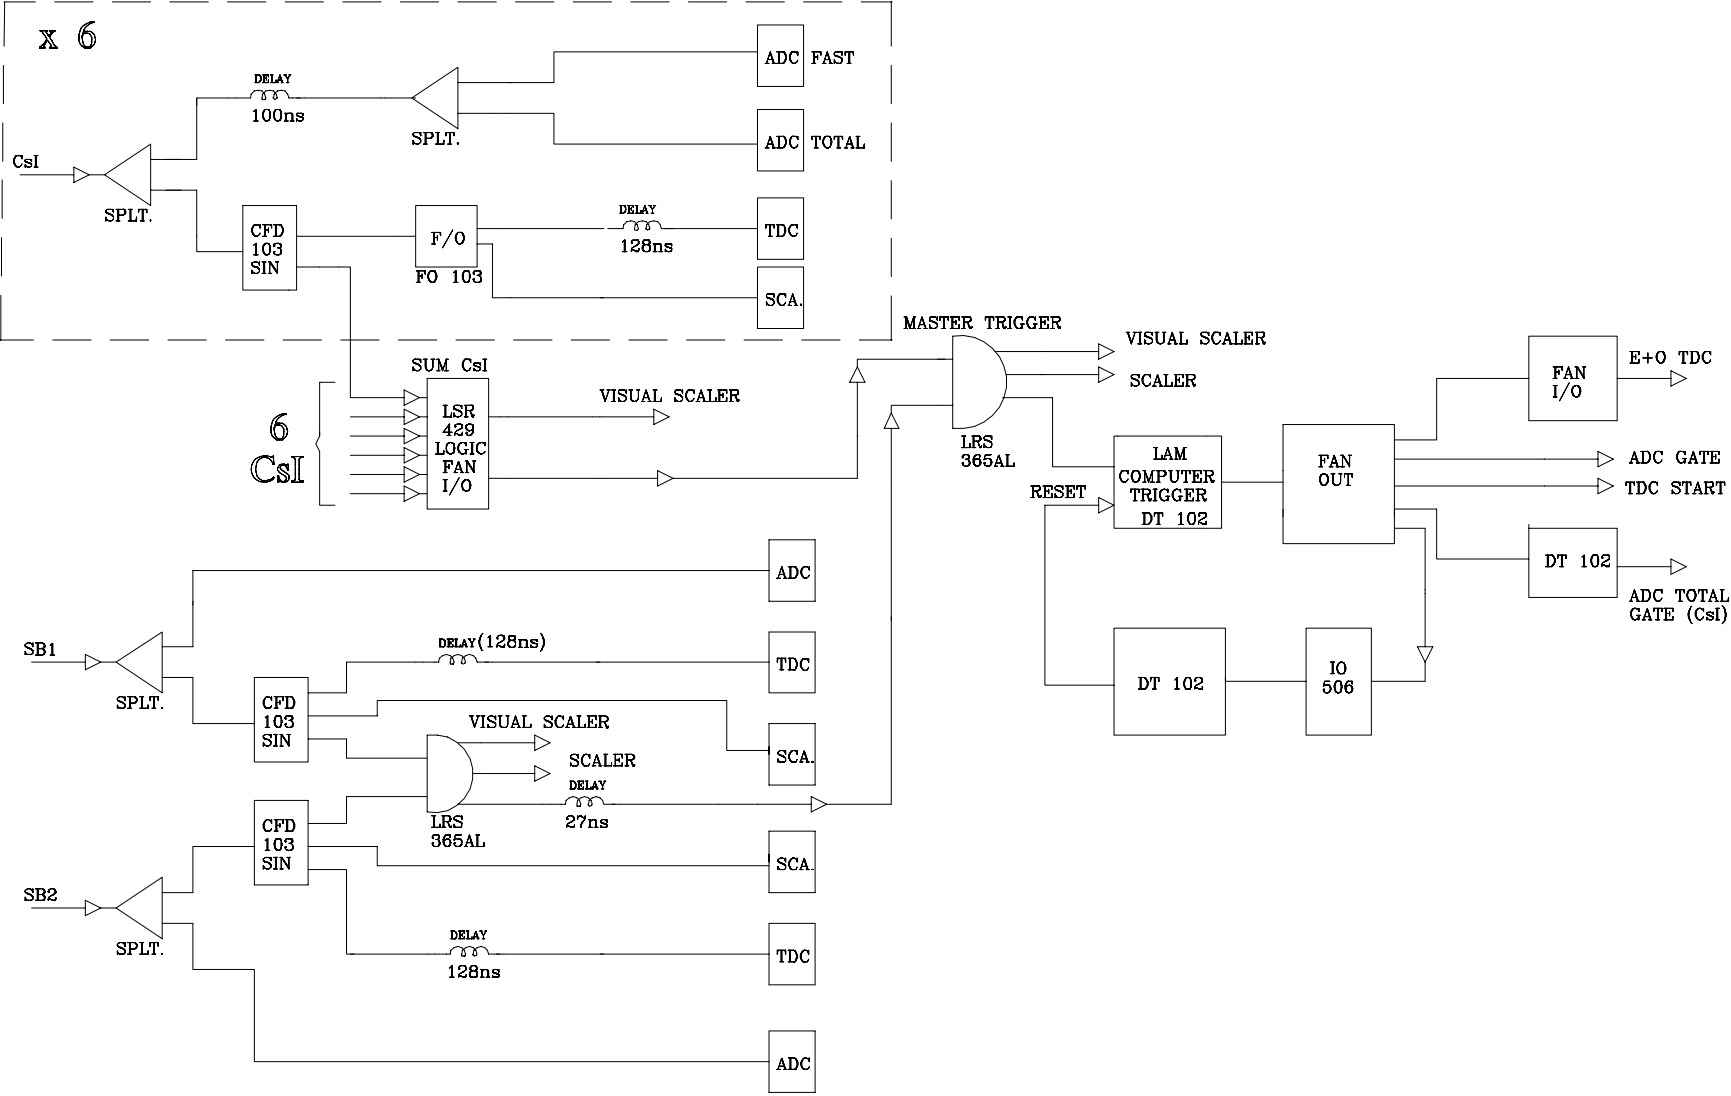

Figure 8.11 Tomography apparatus: trigger electronics. The master trigger is the coincidence of the two scintillator counters of the "OR" of the six modules. For the calibration of the chambers, the trigger reduces to a coincidence of the two scintillators.